

Tinytag Aquatic 2 (-40 to +70°C)

TG-4100

Issue 6
27th November 2009
E&OE

Designed with long term immersion in mind, this unit is waterproof to a depth of 500m making it ideal for environmental monitoring in rivers and oceans. The high visibility yellow case has an attachment point that can be used to secure the logger in position.

The lid can be removed to enable user replacement of the battery.

Data is downloaded to the computer via a USB or serial download pad. This 'wireless connection' eliminates the need for sockets with waterproof caps which can easily be lost or forgotten.

For depths greater than 500m see ACS-0001.

Popular Applications


- Environmental monitoring
 - Fisheries
 - Aquaculture
 - Rivers
- Food Processing



Features

- Submersible temperature recorder
- Waterproof to 500m
- 32,000 reading capacity
- User-programmable logging interval
- 2 user-programmable alarms
- Delayed and trigger start options
- 3 stop options
- User-replaceable battery
- Low battery warning






Features

| | |
|-------------------------------|--|
| Total Reading Capacity | 32,000 readings |
| Memory type | Non Volatile |
| Trigger Start | Magnetic Switch |
| Delayed Start | Relative / Absolute (up to 45 days) |
| Stop Options | When full After n Readings Never (overwrite oldest data) |
| Reading Types | Actual, Min, Max |
| Logging Interval | 1 sec to 10 days |
| Offload | While stopped or when logging in minutes mode |
| Alarms | 2 fully programmable; latching |

Reading Specification

| | |
|---------------------------|--|
| Reading Range | -40 °C to +70 °C (-40 °F to +158 °F) |
| Sensor Type | 10K NTC Thermistor (Internally mounted) |
| Response Time | <20mins to 90% FSD in moving water |
| Reading Resolution | 0.01 °C or better |
| Reading Accuracy | |

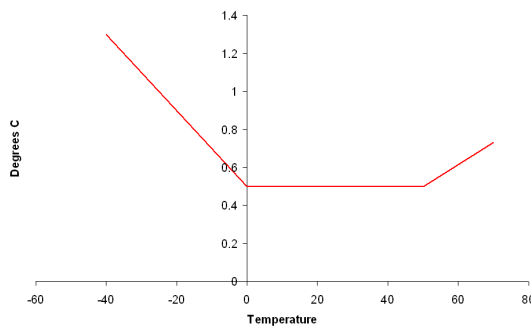

Calibration

This unit is configured to meet Gemini's quoted specification during its manufacture.

We recommend that the calibration of this unit should be checked annually against a calibrated reference meter.

A UKAS traceable certificate of calibration can be supplied for an additional charge either at the point of purchase, or if the unit is returned for a service calibration.

Approvals

This equipment complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) this device may not cause any harmful interference, and (2) the device must accept any interference received, including interference that may cause undesired operation.

Gemini Data Loggers (UK) Ltd. operates a Quality Management System which conforms to ISO 9001. The scope of the system covers the manufacture, design and supply of data loggers and their associated software, accessories and services.



Physical Specification

| | |
|---------------------------|--------------------------------------|
| IP Rating | IP68 water proof (see notes) |
| Operational Range* | -40 °C to +70 °C (-40 °F to +158 °F) |
| Case Dimensions | |
| Diameter | 51mm / 2.01" |
| Height | 50mm / 1.97" |
| Weight | 90g / 3.17oz |

*The Operational Range indicates the physical limits to which the unit can be exposed, not the reading range over which it will record.

Notes

This unit should only be opened when a battery replacement is required.

| | |
|---------------------|----------------|
| Battery Type | Renata CR2450N |
|---------------------|----------------|

| | |
|-----------------------------|-----------|
| Replacement Interval | Annually* |
|-----------------------------|-----------|

*If deployed for long periods, the logger's battery should be replaced annually to prevent the loss of data during a recording run. If the logger is being used frequently, the battery should be changed when prompted by a low battery warning from the Tinytag Explorer software.

Before replacing the battery the data logger must be stopped.

Data stored on the logger will be retained after a battery is replaced.

Please refer to the service kit instruction sheet for battery replacement instructions.

If used at low temperatures the data logger should be allowed to warm to room temperature before it is opened to avoid condensation forming inside the unit.

The IP68 rating is valid only when the unit's lid is securely fitted and is valid to a depth of 500m (1640ft).

The gasket fitted in this unit must be replaced every time it is opened.

The position of the unit's trigger start switch is indicated by the ... marking on its base. The switch itself is positioned on the side of the unit, just above the base-lid join, on the edge indicated. When a magnet is held in the correct location, the status LED will light until the magnet is removed.

LED Flash Patterns

When logging, a status LED is visible through the base of the unit. The flash patterns of this indicator are as follows:

| Flash Pattern | Indication |
|--------------------------------|---|
| 1 flash every 4 seconds | Logging |
| 1 flash every 8 seconds | Waiting to Log (trigger or delayed start set) |
| A double flash every 4 seconds | Alarm limit breached |

Required and Related Products

To use this data logger you will require:

SWCD-0040: Tinytag Explorer software or
SW-0500: Easyview Pro software

and an ACS-3030: USB Inductive Pad

Further related products:

SER-9525: Tinytag Aquatic 2 Service Kit
ACS-3020: Serial Inductive Pad